

## NEW SCIENTIFIC BOOKS

D. C. Heath and Company, New York

LABORATORY MANUAL OF INORGANIC CHEMISTRY AND  
ELEMENTARY QUALITATIVE ANALYSIS. C. C.  
Hedges and H. R. Brayton. 233 pages. \$1.48.Designed for college students who devote from three to  
five hours weekly in the laboratory throughout the year to  
the study of inorganic chemistry. No attempt is made to  
cover the entire field of chemistry; the work outlined is  
sufficient for the time schedule of the student.

D. Appleton and Company, New York

THE EARTH AND ITS RHYTHMS. Charles Schuchert and  
Clara M. LeVene. 385 pp. \$4.00.A book on geology for the non-specialist. There is pre-  
sented a picture of the ceaseless processes of change that  
have molded our planet. Fully illustrated.

David McKay Company, Philadelphia

UNDER SAIL IN THE FROZEN NORTH. F. A. Worsley,  
with a preface by Grettir Algarsson. 295 pp.Being the official story of the British Arctic Expedition  
of 1925, led by Worsley and Algarsson. Though written for  
the average reader, the scientific man will find much inter-  
esting material in the book, particularly the "Geological  
Notes," the "Zoological Report," and the account of the  
hydrographic work.

## THE MICROSCOPE

By SIMON H. GAGE, of Cornell University

Revised, Dark-field Edition (1927) now Available.

The Old and the New in Microscopy, with a special chapter  
on Dark-Field Methods and their Application.

Postpaid, \$3.50

COMSTOCK PUBLISHING CO., ITHACA, N. Y.

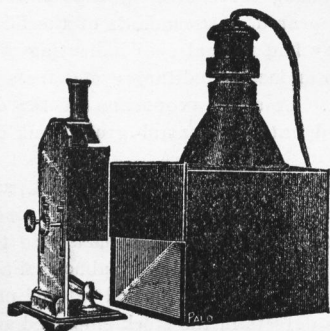
WASHINGTON  
UNIVERSITY  
SAINT LOUIS

## School of Medicine

## NEW ADMISSION REQUIREMENTS

At least three years of approved college  
work including specified requirements in the  
sciences.DEGREE OF B.S. IN MEDICAL  
SCIENCEThis degree may be awarded at the end of  
the third or fourth year to students fulfilling  
certain conditions including the preparation  
of a thesis.

## DEGREE OF DOCTOR OF MEDICINE

Upon satisfactory completion of prescribed  
four-year course.For catalogue and information, address  
THE DEAN, Washington University  
School of Medicine, St. Louis,  
MissouriFor use with Colorimeter; also for  
pH colorimetric work as used by  
Dr. CullenGuaranteed  
DaylightThe Palo lamp illustrated at  
the left produces a duplicate of  
North Skylight, the accepted  
standard for scientific work.The light from a bulb is fil-  
tered through an accurate filter  
lens, the color composition of  
which has been previously deter-  
mined. The resultant North  
Skylight rays are directed upon  
a reflector which increases the  
light diffusion and thus produces  
a more accurate and uniform  
illumination.

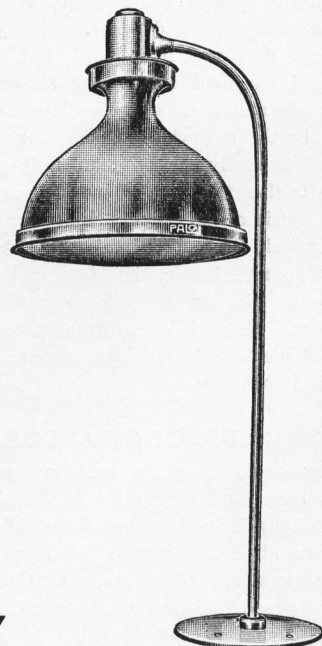
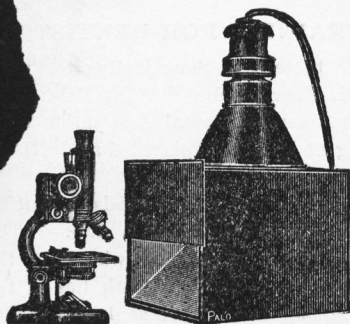
Write for new Daylight Bulletin

## PALO COMPANY

APPARATUS FOR INDUSTRIAL AND  
LABORATORY USE

153 West 23rd Street

New York, N. Y.

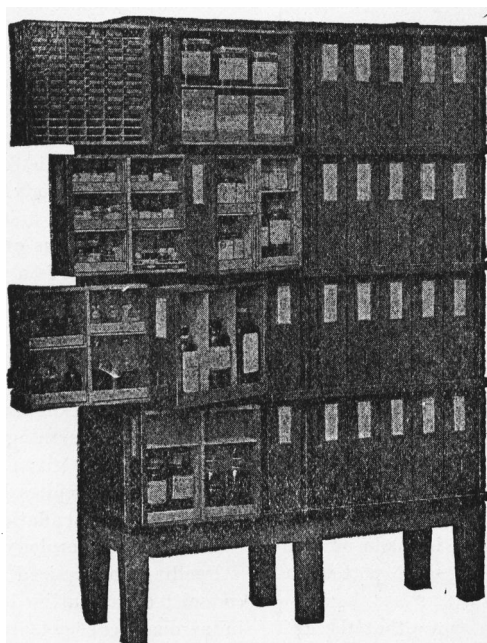
New North Skylight lamp.  
Serves a double purpose,  
both as a table illuminant  
and as microscopic illumi-  
nation for four microscop-  
ists at one time

For Microscopic Use

## You Don't Buy Laboratory Chemicals and Apparatus Just to Waste Them

**T**HE old practice of cluttering up laboratory work tables with valuable chemical reagents and samples is the direct cause of a large proportion of breakage and resultant material losses. Besides breakage, laboratory accuracy is often times affected by congested working space. The Schwartz Sectional System is to the laboratory what the Modern Letter File is to the Busy Office. Containers and apparatus of any size or shape are systematically and scientifically filed in dust-proof drawers which open and swing at an angle that exposes them to view the same as if they were on an open shelf.

The work table is thus kept free from congestion, and the possibility of breakage and loss reduced to a minimum.



Two Vertical Units, one partly open, one closed. With Sanitary Base

Schwartz Cabinets are made in size to suit the needs of the smallest or the largest laboratories, special cabinets are made to fit special spaces.

We index for you all the individual items you file in your Cabinet.

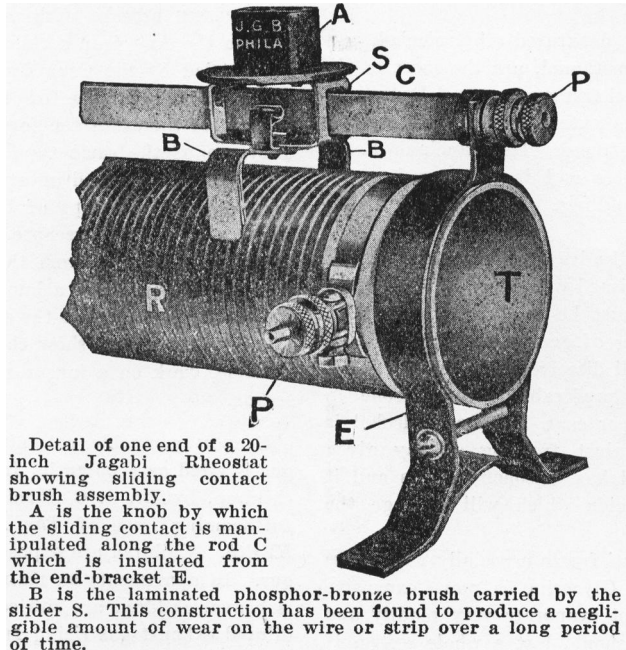
*Write for Booklet "S"*

*Containing Illustrations and Prices.*

## SCHWARTZ SECTIONAL SYSTEM

*Indianapolis, Indiana*

# Important Improvements in JAGABI RHEOSTATS



**JAGABI** Sliding-contact Tube Rheostats are now regularly supplied with certain changes in design which give them greater ruggedness, longer life and added usefulness in their numerous applications. They are:

## "Screw-Drive" Rheostats

We find an increasing demand for Jagabi Rheostats equipped with screw-driven fine adjustment,—an arrangement which has been in existence for many years. We have somewhat re-designed the "screw-drive" making it better adapted to present-day needs. It is described in Catalog 1140-S.

1. An entirely new design of sliding brush contact which is more flexible, is less easily bent out of shape, makes less wear on the resistance wire or strip (which is very important in fine-wire rheostats), and makes a *better* contact.

2. A heavy rectangular slider bar is now used on all 20-inch rheostats, giving greater strength and stability, so that the brush contact cannot be either sprung out of shape or made to cut into a fine winding.

These improvements *have not increased the price* of Jagabi Rheostats, and have been adopted as standard construction only after thorough investigation, test and approval in the most severe service conditions.

Jagabi Rheostats are made in 57 different standardized ratings, which are carried in stock for prompt shipment. These are in three sizes of tubes—20, 16 and 8" lengths, ranging from 30,000 ohms, .1 ampere down to .34 ohm, 25 amperes.

Many special types also are available, including Compression Carbon Rheostats. Write for Catalog 1140-S.

## JAMES G. BIDDLE

ELECTRICAL AND SCIENTIFIC INSTRUMENTS

1211-13 ARCH STREET, PHILADELPHIA

|  |  |                           |               |
|--|--|---------------------------|---------------|
| "POINTOLITE" LAMPS   | SIEMENS & HALSKE PRECISION INSTRUMENTS | OSCILLOGRAPHS             | GALVANOMETERS |
| DIRECT READING OHMMETERS   | "MEGGER" TESTING SETS                  | LABORATORY POTENTIOMETERS |               |
| LANGMUIR CONDENSATION HIGH-VACUUM PUMPS AND OIL-SEALED ROTARY VACUUM PUMPS |  |                           |               |
| LABORATORY AND WORKSHOP RHEOSTATS  | SPEED-MEASURING INSTRUMENTS            | STANDARDS OF RESISTANCE   |               |